

R. Zahoransky  
Wizard Z. KG  
Todtnau  
Germany

**26**

**On-line/in-line measurements  
of particle emissions by optical multi-wavelength technique**

# ON-LINE/IN-LINE MEASUREMENTS OF PARTICLE EMISSIONS OF DIESEL ENGINES BY OPTICAL MULTI-WAVELENGTHS TECHNIQUE

R.A. Zahoransky, E. Laile<sup>1</sup>, B. Terwey<sup>2</sup> and A. Konstandopoulos<sup>3</sup>

<sup>1</sup>WIZARD Zahoransky KG, Schwarzwaldstr. 3, 79674 Todtnau, Germany

<sup>2</sup>Fachhochschule Offenburg, Badstr. 24, 77652 Offenburg, Germany

<sup>3</sup>CE.R.T.H./CPERI, P.O. Box 361, 57001 Themi/Thessaloniki, Greece

## Keywords

Particle emissions, optical on-line/in-line measurements, non interfering measurements

## Abstract

*A system for the on-line/in-line measurement of soot particle sizes and concentrations in the undiluted exhaust gas of diesel engines was developed and successfully tested. The unit uses the individual attenuations of three different laser wavelengths and is combined with an optical cell (white principle) with adjustable path lengths from 2.5 to 15 meters.*

## 1 Introduction

Sharpened European and national regulations for the exhaust gas of diesel engines demand improved particle measurement systems for the periodic inspection and particle analysing tools for enhanced motor developments.

The importance of getting also a size information along with the concentration values has grown up with the up-coming discussion of the health effects of soot emissions.

The presented measurement system delivers both: Size and concentration information directly retrieved from the undiluted exhaust gas from vehicles on a chassis dynamometer and also from engines on motor test benches.

## 2 Measurement unit

The sensor head (Fig. 1,2) contains three laser diodes of different wavelengths which are combined in one focussed beam. The spectral attenuation of the three wavelengths is captured at a single detector and the particle diameter and concentration is evaluated by the use of the Mie theory [1] and shown on-line with the speed of 1 Hz.

A commercially available optical long-path-cell (Fig. 3, white principle) was modified with a new developed purging and flushing system. This unit has a base path length of 62.5 cm, and allows an adjustment of the optical path length from 2.5 to 15 m by a mirror system.

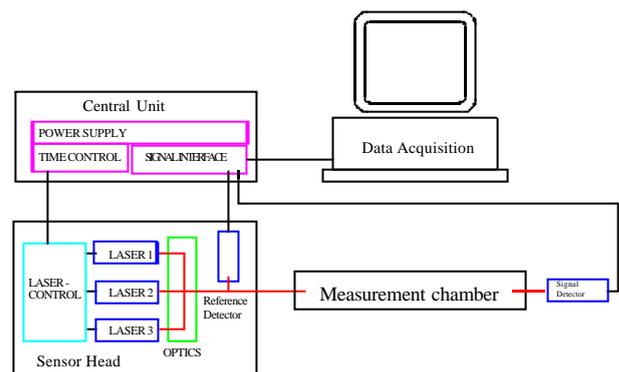


Fig 1: Schematic of the new sensor



Fig. 2: Sensor head with supply and interface unit



The measurement cell and the exhaust gas tubes are heated and thermo-controlled to avoid conflicts with deposition and interferences by condensation i.e. formation of water droplets.

Temperatures and pressures are recorded to allow the calculation of standard conditions.

The use of the long-path-cell enlarged the dynamic range of measurable concentrations compared to previous measurements within a long tube [2,3] so effectively, that also measurements at engines with filter after-treatment systems are intended.

Fig 3: Sensor with optical

Fig. 3 shows the sensor, consisting of the signal detector and the transmitting unit adapted to the long-path-cell at the bottom side.

### 3 Results

The on-line graphs in Fig. 4 contains the whole aerosol information:

- ① Mean Diameter:
- ② Volume concentration
- ③ Raw intensities of the three lasers
- ④ Theoretical field

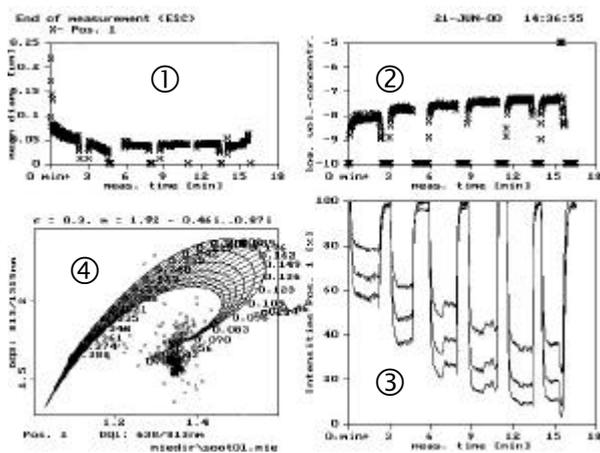


Fig. 4: On-line graph of the system

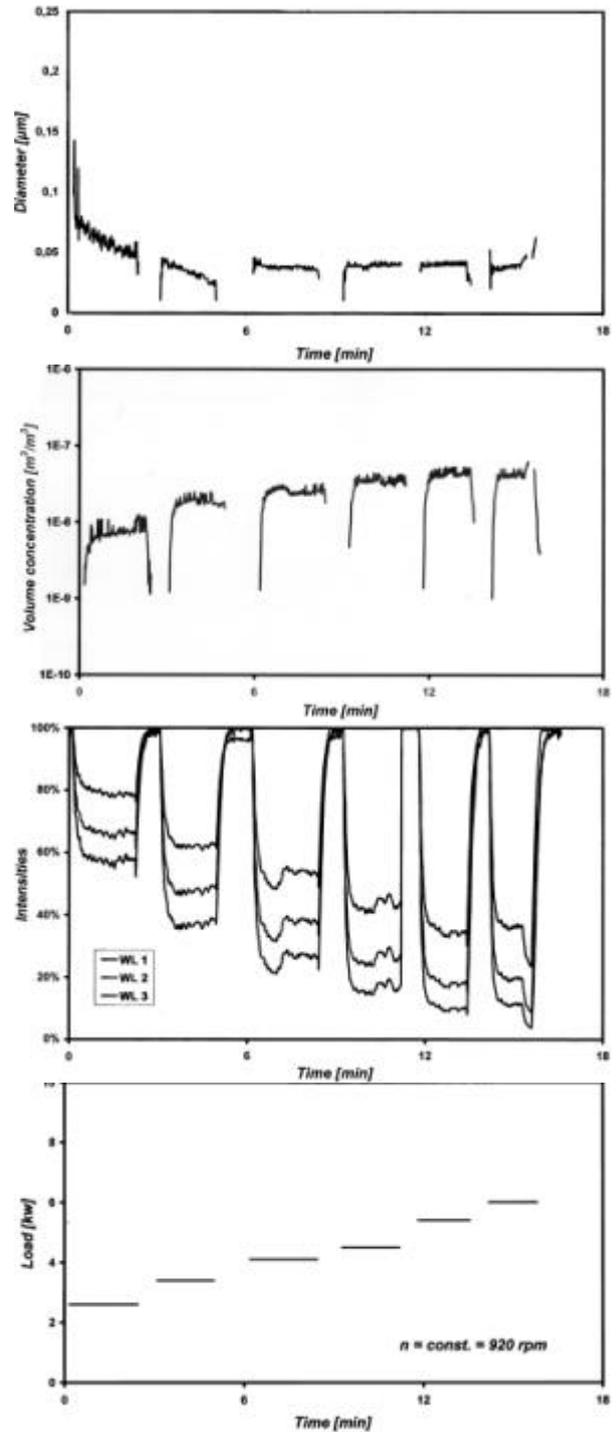


Fig. 5 a-d: Results of an AUDI 1,9l TD on a chassis dynamometer

Fig. 5 shows the detailed results of this specific measurement. Different loads, starting with idle conditions, under constant speed of rotation are recorded for an AUDI 1,9l TD on a chassis dynamometer (Fig. 5d).

The graphs show clearly that the mean diameter of the emitted particles are well below 100 nm (Fig. 5a). The Mie calculations are based on the assumptions of a log-normal distribution and spherical

particles. If chain like agglomerates are present in the aerosol, this optical system measures in good agreement with REM images the diameter of the spherical primary particles.

In some older engines, a correlation between engine's load and emitted particle size was found. This correlation is not so clearly manifested in modern engines with direct injection or exhaust gas recirculation. Further investigations are under way.

As expected, the concentration (Fig. 5b) follows the engine's load increase. The load was enlarged stepwise, interrupted by manually activated reference measurements.

Fig. 5c clearly demonstrates the different extinction characteristics of the individual wavelengths in the soot aerosol.

The on-line presentation of the measured values in the theoretical Mie field indicates the quality of the actual results (Fig. 4, ④). It was found, that a refractive index of  $n = 1.92 - 0,66i$  delivers best results for all diesel engines.

In earlier examinations the correlation of the used measurement principle (with this refractive index) to traditional gravimetric and opacity measurements was confirmed [4]. The experimentally found soot density of  $\rho = 0.55 \text{ g/cm}^3$  is also approved by other literature [5].

## 4 Conclusion

The particle analyser based on the optical multi-wavelength extinction proved to be a most reliable tool to measure on-line and in-situ directly the undiluted particle emission of diesel engines. The two main aerosol parameters „mean diameter“ and „volume concentration“ are recorded in the on-line mode.

Advantages of the new measurement system are the use of undiluted exhaust gas and the fast adaptation to engine systems by a simple thermo-controlled hose. The on-line capability permits the measurement of either stationary or transient motor conditions.

A white cell is mandatory for modern diesel engines: An adjustable optical path length of up to 10 m allows the analysis in a sufficiently broad concentration range.

Further developments in extending the features to record representative gaseous species in the exhaust gas are in progress [6,7].

## 5 References

- [1] U. Pfeifer, S. Zarske, W. Samenfink, R. Dittmann, E. Laile, R. Zahoransky  
Optisches Multiwellenlängen-Extinktionsverfahren - angewandt zur on-line Messung der Größe und Volumenkonzentration von Partikeln im Abgas von Dieselmotoren; In: VDI Bericht 1189 (1995)
- [2] R. Zahoransky, W. Kuhnt, E. Laile;  
In-line Particle Measurements of the Undiluted Exhaust of Combustion Engines by Multi-Wavelength Extinction Technique;  
J. Aerosol Sci., Vol. 28, Suppl. 1 (1997)
- [3] R.A. Zahoransky, H.W. Kuhnt, E. Laile, G. Poss  
Particle Emission of Internal Combustion Engines under Transient Load Conditions - on-line Analysis of Particle Size and Concentration by Optical Extinction  
J. Aerosol Sci., Vol. 29, Suppl. 1 (1998)
- [4] Joint research project of the Abgasprüfstelle Berlin-Adlershof GmbH, University Karlsruhe and WIZARD Zahoransky KG  
Dynamisches on-line Verfahren zur Messung der Partikelgrößerverteilung im Abgas von Dieselmotoren (finanziell unterstützt durch die Deutsche Bundesstiftung Umwelt)  
Final report 1994
- [5] E. J. Bissett  
Mathematical model of the thermal regeneration of a wall-flow monolith diesel particle filter  
Chem. Eng. Sci. 39, 1984
- [6] EU CRAFT Contract BRST-CT98-5537;  
MULTISENS Multiwavelength Sensor for Sub-Micron Particle Analysis  
Entwicklergemeinschaft Foundation of Res. & Techn.-Hellas/Chemical Proc. Eng. Res. Institute, WIZARD Zahoransky KG, NOTOX Int. A/S, Obernosterer Strickstoffe GmbH, G.Kechagias-I.Limnidis&Co., Aristotle University-AUTH, project start 1999
- [7] EU RTD (5th Framework Programme); Contract Nr. GRD1-1999-11154  
Particulate Size and Composition Measurements for Diesel Exhaust Aftertreatment PSICO-DEXA  
Entwicklergemeinschaft Foundation of Res. & Techn.-Hellas/Chemical Proc. Eng. Res. Institute, FIAT Auto SpA, WIZARD Zahoransky KG, FEV Motorentechnik GmbH, AVL List GmbH, European Joint Research Center, Istituto Motori/Nat. Res. Council of Italy, Università di Napoli, Clausthaler-Umwelttechnik-Institut GmbH, project start 2000